

## **Operating Instructions for ELIT 4 & 8-Channel Ion Analysers**

First Public Version CCR/HK/YYC 20 May 2003, Last Update: CCR, 21 April 2010

Please see separate **Electrode Operating Instructions** for how to use Ion Selective Electrodes



### **CONTENTS**

#### **A) Introduction**

#### **B) Software Installation**

- 1) System Requirements
- 2) Running Setup Programme from CD ROM

#### **C) Hardware Installation**

#### **D) Software Operation**

- D1) Setup Screen
- D2) Calibration Procedure
- D3) Sample Measurement
- D4) Data Recording and Viewing

#### **E) Exporting Data to other Software**

#### **F) Closedown**

### **A) INTRODUCTION**

This software is capable of recording up to 100,000 data points and must be used with a computer using Windows 2000 or Windows XP operating system.

Tested on :Windows 2000 (English) + Service pack 2 + Patches up to the released date. Windows XP (English) + Service pack 2 + Patches up to the released date.

All the Service Packs can be downloaded free from [www.microsoft.com](http://www.microsoft.com)

**Important:** The software must run on the Windows' English platform, which uses a Decimal Point instead of a Comma to separate the decimals.

If the computer has been setup for using non-English platform, please change the Language to English (United Kingdom) in "Control Panel/Regional Options"(in Windows 2000) or in "Regional and Language Options" (in Windows XP).

The Ion Analyser can be connected to any type of Ion Selective, pH or Redox electrode which has a BNC connector. The software contains several Help files and on-screen hints and warnings which duplicates much of this manual and should enable the operator to perform the analyses easily and reliably.

NB: If only the mV data is required, irrespective of which sensor is connected, then "Redox" must be selected from the drop down boxes in the appropriate channels on the Setup screen. You can then proceed directly to the measurement screen without having to calibrate the electrodes first, and mV will be plotted against time on the graphical output.

**For 4 Channel operation, please ignore any references to channels 5 to 8.**

## **B) SOFTWARE INSTALLATION**

**1) System Requirements** – Please see last page

### **2) Running Setup**

Insert the software disc into the CD-ROM drive of your computer.

The installation (Setup) software should then run automatically – simply follow the on-screen instructions.

If the installation fails to start when you insert the CD, go to My Computer and double Click CD-ROM disc (Usually the D drive unless a second hard drive is installed) or Click on Start and then Run D:\Setup.exe, then follow the on screen instructions.

The running executable file for the 32 bit version is: 4-chan32.exe or 8-chan32.exe

When installation is completed you will be given the option to create a new icon on your desktop. Double clicking on this will start the programme.

## **C) HARDWARE INSTALLATION**

**C1)** Connect the interface to the Serial (COM1) port of the computer (or to any USB port via a USB/Serial Adaptor) using the cable provided.

Connect the mains adapter to an appropriate power outlet.

Note that if a USB/Serial adaptor is used then, after installing the adaptor software, and connecting the interface cable, the USB port must be set to COM1 as follows:

- 1) Open Device Manager by right-click on My Computer icon (on Desktop) and select Properties / Hardware / Device Manager. OR click Start / Control Panel / System / Hardware / Device Manager.
- 2) Then double-click Ports and right-click Prolific USB... Note that Ports option will not appear in Device Manager unless the interface cable is connected !
- 3) After right-clicking Prolific USB... select Properties from the drop-down menu, then Port Settings / Advanced.
- 4) Click on the drop-down box and select COM1 / OK. If there is a message about COM1 being used by another device, ignore it and click yes – change anyway. Then close the Properties window and return to Device Manager.
- 5) Again right-click on Prolific USB ... but this time select Scan for Hardware Changes. This will confirm COM1 as the setting for the USB/Serial adaptor.

**C2)** If you are using ELIT 8mm ISEs with ELIT 8mm Reference electrodes housed in ELIT electrode head system you must connect the electrodes to the interface using the BNC plug(s) attached to the electrode head(s). Similarly, any conventional combination electrodes must also be connected to the BNC connectors. However, if you wish to use separate conventional reference electrodes then these can only be used for channels 1 to 4 and must be plugged into the 2mm jack-plug sockets provided.

**C3)** If simultaneous pH and ISE measurements are required in the same solution then the ISE must be connected without a separate reference electrode. In this case both the ISE and the pH voltage is measured relative to the internal reference system of the standard combination pH electrode. But note that pH electrodes generally cause a slight contamination of the test solution with K, Cl, and traces of Ag because of slow leakage of the filling solution of the reference system through the liquid junction. Thus simultaneous pH measurement may cause anomalous high readings in the measurement of low concentrations of ions for which K, Cl or Ag is a significant interfering factor: e.g. K, Cl, Ag, NH<sub>4</sub>, NO<sub>3</sub>, Cd, ....

**C4)** A maximum of four temperature probes can be connected to the appropriate sockets on the front panel of the interface, and any one of these can be selected to monitor the temperature changes corresponding to any of the electrode channels.

## D) SOFTWARE OPERATION

### D1) Setup Screen.

**4-Channel Ion-Analyser: Setup**

Help

COM Port Setting: Communications Port COM1

Project Details  
Project Name: Test leakage from pH electrode  
Analyst: Chris

Signal Averaging Number  
For Calibrating: 10  
For Measuring: 10

Electrode Properties

Chan.	1	2	3	4
Primary Electrode Details				
Type	Redox	H (pH)	K	Cl
S/N	52311	52322	5501	5502
Reference Electrode Details				
Type	None	Combination	None	None
S/N	None	R6318		
Temp. Sensor				
	None	None	None	None
Calib. Date				

Calibrate Calibrate Calibrate Calibrate

Simultaneous Calibration

Measure > View Data File Exit

9:42:27 04.Apr.2007

**4-Channel Analyser** for 4 Electrodes and 4 Temp. Sensors using any combination of pH, Redox or ISEs.

**For measuring in several different vessels simultaneously** - each sensor electrode has its own separate reference electrode.

**For simultaneous multi-component analysis in a single vessel** - all sensors use the same single reference electrode - but be sure to check that the various ions to be measured do not interfere with one another.

If pH is required together with ISE and/or Redox, a standard combination pH electrode is used to provide the reference system for all the other mono-electrodes; this may not be suitable for ions where K and Cl are interferences, particularly at low concentrations.

**Note that for 8-channel operation, channels 5 to 8 are displayed in place of the analytical notes.**

**D1a)** The first screen allows you to enter all the details necessary for setting up your experiment / measuring system and producing a complete documentation for archiving and GLP procedures.

Most of this should be self-explanatory. If any of the required data is not available, e.g. electrode serial numbers, then the software will accept any single character or groups of characters as a default. Move the cursor using the Tab key or click with the mouse.

NB: You will not be able to proceed to the Measuring screen until all relevant data is entered here, including calibration. Thus, if only the mV data is required, irrespective of which sensor is connected, then "Redox" must be selected from the drop down boxes in the appropriate channels on the Setup screen. You can then proceed directly to the measurement screen without having to calibrate the electrodes first, and mV will be plotted against time on the graphical output.

**D1b)** The **View Data File** button at the bottom of the screen will give immediate access to old stored data files for review and printing without having to go through any of the

setup procedures. See section D4 in this manual and the View Data Help file in the software for details.

**D1c)** The **Port Setting** box has a normal default for the interface to be connected to Serial Port (COM1) of the computer and you must make sure that this is correct for your setup.

**D1d)** The **Signal Averaging Number** is the number of readings to be taken (at 2 second intervals) and averaged to produce the final value for the millivolts produced by each electrode. The higher the number of readings, the more stable and precise the measurement.

The value displayed on the screen is the result of a 'gliding average' which produces a stable value which is the average of a number of readings but is updated frequently as each new reading is taken.

## **D2) Calibration Procedure.**

**D2a)** Once the Hardware Setup has been completed and the correct electrodes have been allocated to the appropriate channels they must be calibrated with standard solutions of known concentration (or pH) before being used to measure unknown sample. This can be done individually, if a number of different electrodes are being used (click on the appropriate **Calibrate** button), or simultaneously for any number of identical channels (use **Simultaneous Calibration**).

### **Operational notes:**

1) For the most accurate stable measurements with ISEs it is recommended to wait at least 2 minutes after the ISE is immersed in the sample or standard before taking a reading. Low concentrations (below 1 ppm) may take up to 10 minutes to reach a completely stable reading. It is also useful to increase the Signal Averaging Number (see D1d, above) to 10 to 30, which means the system takes 10 to 30 measurements at 2 second intervals and displays the average of these measurements. This procedure reduces the influence of electromagnetic noise and chemical instabilities. For fast measurements when highest precision is not required, the waiting time and average number can be reduced.

2) Calibration is not required for Redox electrodes which simply record the measured voltage. After assigning Redox to a particular channel, click **Measure** to start data recording.

3) Once a channel has been calibrated, the data are stored for later use and the time and date of the calibration is recorded above the Calibrate button. The next time the software is used it is then possible to go straight to the Measure screen without performing a new calibration. However it must be stressed that this facility is only recommended for making a rough check before starting a completely new batch of samples in order to find the best range for the new calibration standards. Large errors can be introduced if you start a new batch of samples on a new day (or even a few hours later) without making a new calibration.

**D2b)** For individual calibrations you are presented with a calibration window in which you must select the number of calibration solutions (default is 2, maximum 6) and the concentration units you wish to use. To define the slope of the calibration graph, you must use at least two standards, preferably spanning the range of concentrations in your samples. If the sample range is greater than one order of magnitude then it is



Clicking on **Finish** again will return to the main **Setup** screen. Selecting **Finish** at any other time will give you the option to return to the main screen without completing the calibration.

**D2h) Simultaneous Calibration** works in the same way, except that you are initially presented with a table from which to select which channels to calibrate at the same time. During calibration, you need only type the concentration once and must immerse all the electrodes in the same solution at the same time.

**D2i)** Selecting **Calibrate** for an electrode which has already been calibrated will reveal a summary of the existing calibration data.

**Calibration Summary**

Electrode Type: Cl  
 Located Channel: Channel Two  
 Last Calib Date: 15:09:37 11.Mar.2002

Calibration Points: 4

Standards:	Concentration (ppm)	mV	Slopes
1.	1	234.6	-43.6
2.	10	191	-53.1
3.	100	137.9	-55.1
4.	1000	82.8	

Buttons: Continue, Help, Finish

Background interface elements:  
 Calib. Date: 11.Mar.2002 11.Mar.2002 N/A N/A N/A N/A  
 Buttons: Calibrate, Simultaneous Calibration, Measure >, View Data File, Exit  
 Status bar: 15:18:22 11.Mar.2002

### **D3) Sample Measurement.**

**D3a)** Once calibration has been completed for all the channels to be used, the sample measurement screen is accessed by clicking on the **Measure** button. **It is important to note here that all sample measurements should be made in exactly the same way as standards, e.g.: same waiting time, Average Number, stirring conditions, temperature etc.**

For repeated measurement of different samples, data are recorded manually, at the click of a button. Alternatively, for continuous process monitoring of the same solution, data can be read automatically. In this mode the interval (in seconds) between each measurement must be entered in the **Frequency** box, after selecting **Automatic** from the drop-down menu.

**D3b)** On first entering the screen there is a short delay, and the data channels are blank, whilst the interface takes the first set of readings, but thereafter there is a continuous display of the voltage, the calculated concentration (in ppm and moles, or pH) and temperature, if appropriate.

**D3c)** to make a manual sample measurement, ensure that **Manual** Data Recording is selected from the drop down menu, immerse the electrode(s) in the appropriate solution(s), wait for a stable millivolt reading (or for a specified time) and click on the **Record** button

The first time **Record** is used you will be presented with the standard Windows 'SaveAs' box in which you must create a file name in which to store the data. Thereafter, each time you click **Record**, the data will be automatically saved in this file.

If you wish to enter any sample numbers or comments to accompany this set of data then these must be typed into the **Comment** line before clicking on **Record**.

ELIT 4-Channel Ion-Analyser : Data Acquisition

Help

Project Details  
Project Name: Test 1  
Analyst: Chris

Measurement Details  
Data Record Mode: Automatic  
Frequency: 10 Sec.  
Stored Records: 0

\* Sample Measurement \*

Channel:	1	2	3	4
Prime Elect. Type:	Redox	Redox	Redox	Redox
S/N:	52311	52322	52323	52324
Ref. Elect. Type:	None	None	None	None
S/N:	None	None	None	None
mV:	0.0	0.0	0.0	0.0
pH:	N/A	N/A	N/A	N/A
ppm:	N/A	N/A	N/A	N/A
mol/l:	N/A	N/A	N/A	N/A
Temp. Sensor:	None	None	None	None
Temp. Celsius:	N/A	N/A	N/A	N/A

**Data Acquisition 4-Channel Analyser:**  
Data can be recorded Manually or Automatically. If Manual is selected then data is recorded each time 'Record' is clicked. In Automatic mode the frequency of measurement can be selected.

**Data can be displayed in Graph or Table:**  
Clicking 'View Data File' on the previous Setup screen (for existing data) or Data Acquisition screen, (for new data). Data also can be viewed in 'real time' when using automatic data acquisition. Data can be displayed mV, pH, ppm, mol/l, or Temp and select using any combination of channels.

Comment : Demonstration display only - no data input ||

< Back   Record   Average Number   View Data File   Exit

9:50:53 04.Apr.2007

**D3d)** Alternatively, for continuous process monitoring in automatic mode, simply immerse the electrodes in the appropriate test solutions and click on **Record** and, after creating a data file, the data will continue to be read and saved at the specified time interval until you click **Stop**. Comments can be added during data acquisition by clicking on **Stop**, typing in the comments, then clicking on **Record** again – or they can be added to the data table later using the **View Data File** facility.

**D3e)** A counter in the **Stored Records** box continuously displays the number of data lines in the current data file.


**D3f)** If necessary, the **Average Number** can be changed during manual sample measurement. (see section D1d)

**D3g)** At the end of a measurement session you can either go **Back** to the calibration/setup screen or click **Exit** to close the programme.

#### **D4) Data Recording and Viewing**



**D4a)** The saved data can be viewed at any time using the **View Data File** button - but note that initial use of this function, during data acquisition, will require the **Update/Update Now** option from the tool bar to be activated before the current data file will be displayed.

**D4b)** The data are initially displayed in graphics mode. This shows the electrode output plotted against the data number for all active channels. The output from individual electrodes can be plotted separately or any combination can be shown together by choosing **Chan Selector** from the **View** menu. There are options in **Chan Selector** to plot mV, pH, ppm or moles/l as appropriate and you can also choose to plot the output from the temperature sensors. **Update** has an **Automatic** option which permits continuous and simultaneous display of the change in signal in all the selected channels during automatic data acquisition.

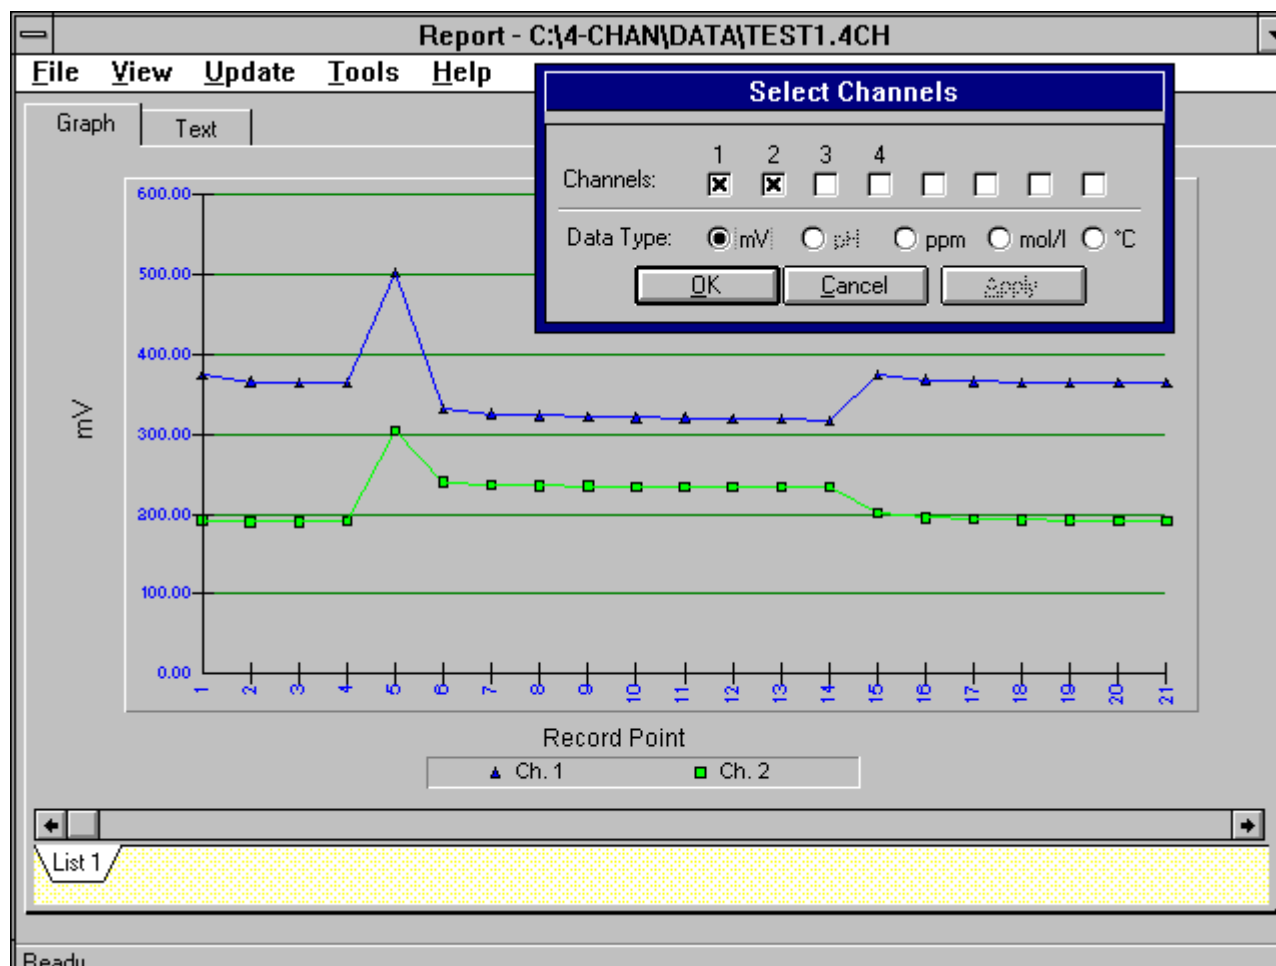

**D4c)** The graphics screen will display up to 50 data points at a time. During Automatic Recording, this will automatically jump forward in blocks of 50. If viewing of earlier data is required then this can be done by switching off the automatic update option (re-click on **Automatic**) and then using the scroll bar at the bottom of the screen. Note that a message in the title bar will inform you of the last data point to be plotted as the scroll box is dragged along the bar. Note also that this will only stop the automatic data display update – the data acquisition and saving will not be affected.

**D4d)** The graphics screen also includes several standard graphic tools to enable the operator to produce a customised display (including changing scales, inserting ticks and labels, producing 3 D bar charts, etc etc.) - these are available via the Graph Control window which is opened by clicking any of the graph Icons above the display. Once you are satisfied with the re-formatted graph, click on the "System" Tab in Graph Control window and type a new file name in the Graph Template File "Browse" box - NOT the "Name" box! This file name can be the same as the original .4ch data file if you wish. Then be sure to tick the "Save Data" box before clicking on Save. The file will be saved with a .gsp termination in the same folder as the .4ch data files.

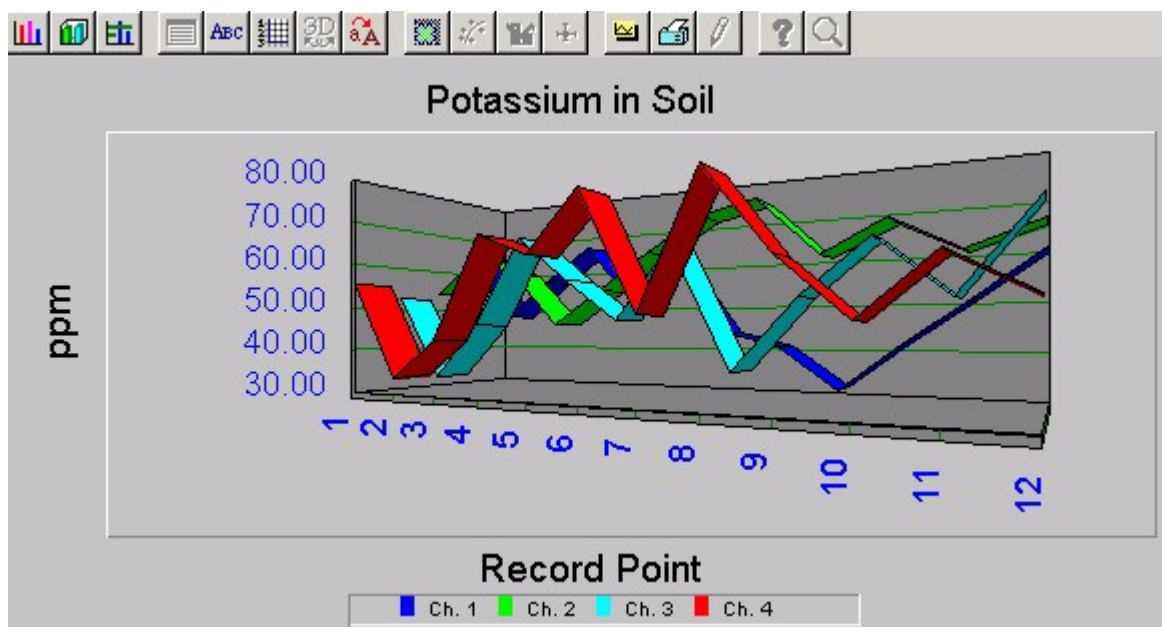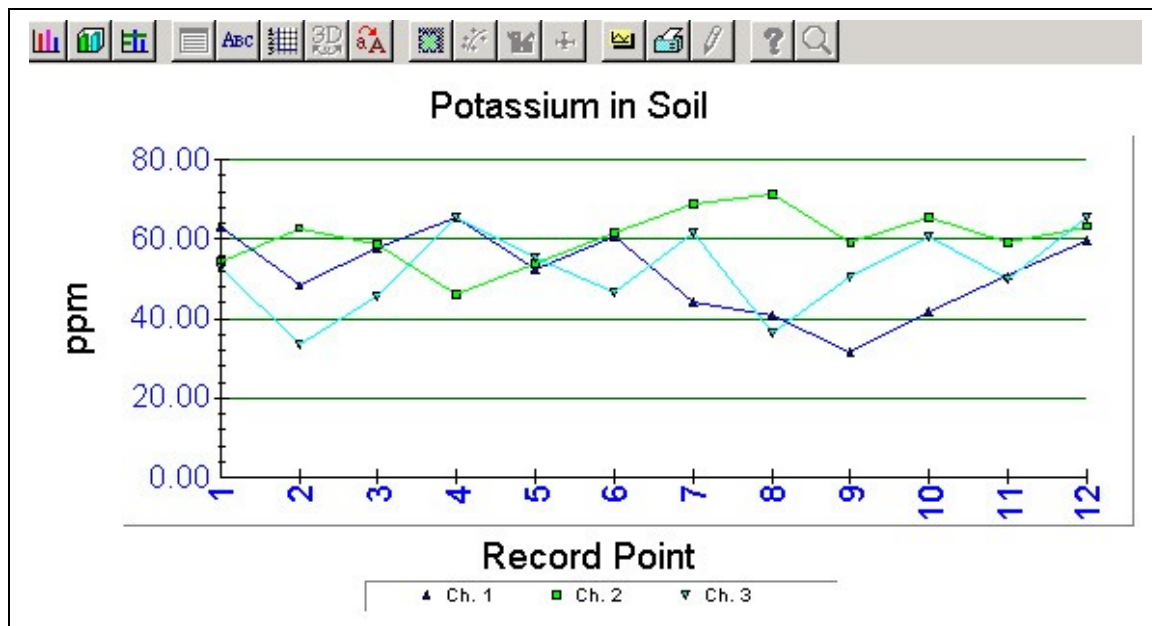



To retrieve this file for later modification, printing or exporting, Click View Data Files / File / Open and select the original .4ch data file. When this is open, click any graph icon (or, specifically, the green printer icon fourth from the right) to open the Graph Control and select the System tab. Then Browse the Graph Template File box or type in the file name and click "Load".

If you want to save this graph as an image file then check the Image/Bitmap and Target/File buttons under the Export label and then click Browse. You will then be

presented with a standard Save As window where you can type/select the file name and destination folder for the image. This can then be converted to, for example, .gif or .jpg format using standard image handling software.

**D4e)** The data can also be viewed in tabular form by clicking on the **Text** label and using the vertical scroll bar to select particular lines. Note that each data table will only take about 4000 records, hence the **List1** label. When this is exceeded, a new table is started with a new **List** label.

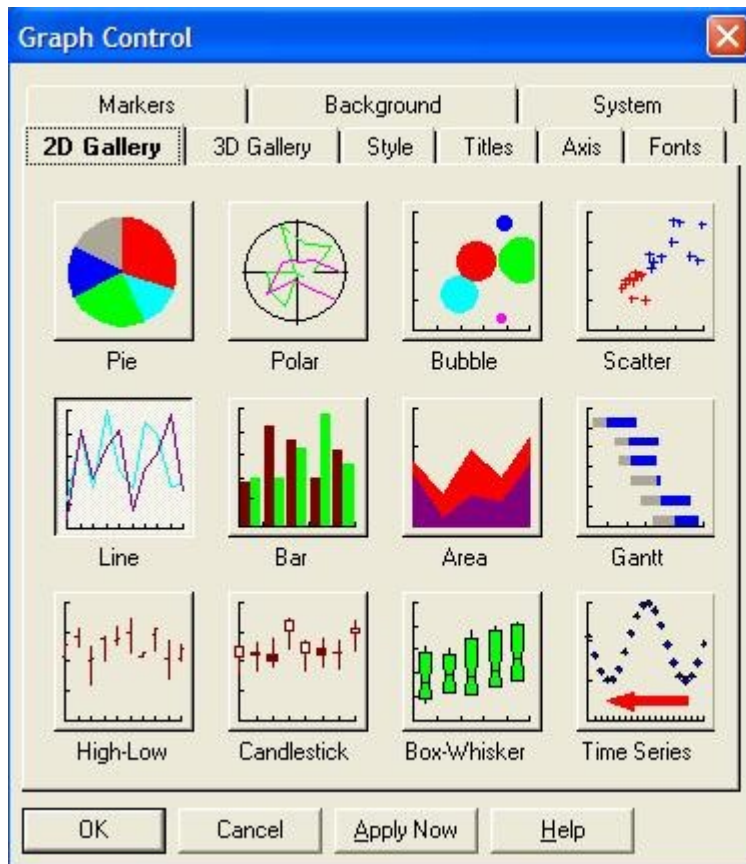

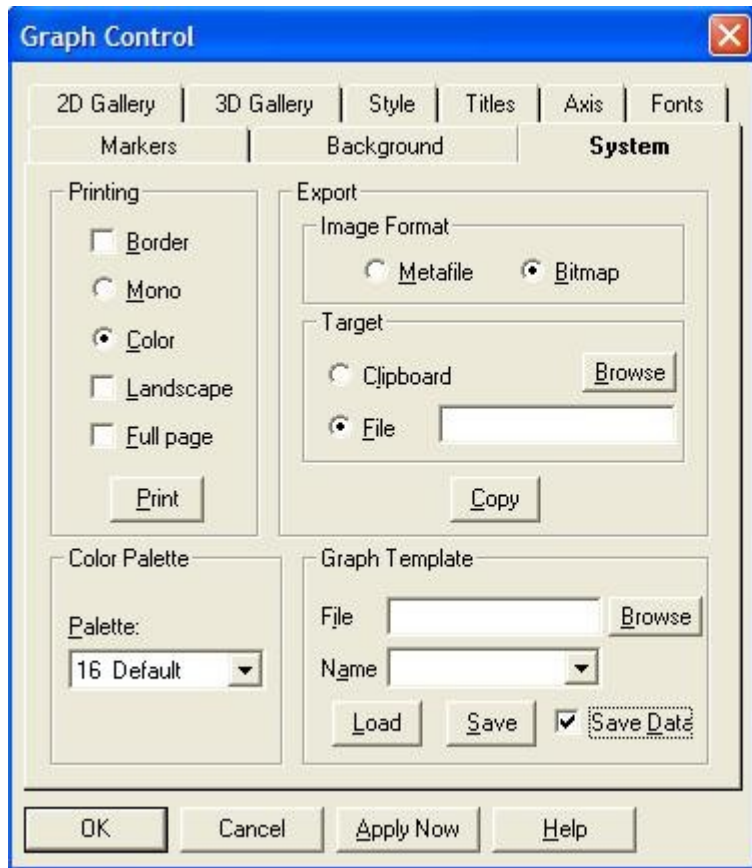

**Report - C:\4-CHAN\DATA\TEST1.4CH**

**File View Update Tools Help**

Project Name: test K and Cl stabilisation      Report Created At: 15:23:21 11.Mar.2002  
 Analyst: chris

	Chan 1	Chan 2	Chan 3	Chan 4	Chan 5	Chan 6	Chan 7	Chan 8
Electrode :	K	Cl	Redox	Redox	None	None	None	None
Serial No. :	1234	2345	3456	4567				
Ref. Type :	LiAc	LiAc	None	None	N/A	N/A	N/A	N/A
Ref. S/N :	1234	2468						
Temp. Sens. :	1	1	N/A	N/A	N/A	N/A	N/A	N/A
<b>Slopes Info.</b>								
Slope 1:	51.5	-43.60001	N/A	N/A	N/A	N/A	N/A	N/A
Slope 2:	50.30002	-53.10001	N/A	N/A	N/A	N/A	N/A	N/A
Slope 3:	45.69998	-55.09999	N/A	N/A	N/A	N/A	N/A	N/A
Record 1	At	15:23:21 11.Mar.2002						
Comment:								
mV	375.1	192.3	376.4	192.3	N/A	N/A	N/A	N/A
ppm	27.6	9.7	N/A	N/A	N/A	N/A	N/A	N/A
mol/l	7.05E-04	2.74E-04	N/A	N/A	N/A	N/A	N/A	N/A
°C	56.8	56.8	N/A	N/A	N/A	N/A	N/A	N/A
Record 2	At	15:23:31 11.Mar.2002						
Comment:								
mV	365.8	190.6	366.0	190.6	N/A	N/A	N/A	N/A
ppm	10.9	10.1	N/A	N/A	N/A	N/A	N/A	N/A
List 1								

Ready

**D4f)** Individual records can be quickly accessed by record and channel number using **Record Search** from the **Tools** menu. This menu also gives quick access to the Windows **Calculator** and **Notepad**.

**D4g)** Choose **File/Close** to exit the View Data File screen.

**D4h)** Old data files can be reviewed using **View Data File** from the setup screen or from the data acquisition screen. Choose **File/Open** to see all existing data files.

**D4i)** Once a data file has been opened, **File/Print** will allow you to print either the current data table (click on **Text**) or the graph. Note that the graphics printing is limited to a maximum of 1500 data points (ie. number of records times number of channels), thus for large data sets it is important to choose a limited range of records (rather than **All**) before trying to print the graph. Note also that for large data sets, **Print/Text** will only print the current **List**. Thus, for a full data printout, each List must be selected and printed individually.

## **E) EXPORTING DATA TO OTHER SOFTWARE:**

Data are stored in ASCII text files which can be read by other applications such as MS Notepad or Excel etc. The files have an operator defined name and a .4ch or .8ch extension: e.g. Test1.4ch or Test2.8ch. They are normally saved in C:\Program Files\4( or 8 )Channel Interface(32)\Data\ (unless the initial installation was made into a different folder).

**WARNING:** If you wish to save a data file in a new format, remember to use Save As to save it with a different name or in a different folder - to avoid confusion and avoid corrupting the original file.

For Example: to open with Notepad, first launch Notepad then click File/Open and select "Any File". Find the folder and the file you wish to open and double-click it.

To open with Excel, launch Excel and follow the procedure above to find the file. In this case, on double clicking the file name, you will see the "Text Import Wizard", where you must select "Delimited", then click on Finish.

## **F) CLOSEDOWN**

The software can be closed down by choosing Exit from the Data Acquisition or Setup screens or by double clicking on the " x " box in the top right hand corner of the screen.

**SYSTEM REQUIREMENTS:****Win2000:**

Computer/Processor: 133 MHz or higher Pentium-compatible CPU.  
128 megabytes (MB) of RAM or higher recommended (64 MB minimum supported; may limit performance and some features)  
500 MB available hard disk space  
CD-ROM or DVD drive  
Display: VGA or higher resolution monitor.  
One free COM port  
Keyboard and mouse are required.

**WinXP:**

PC with 300 megahertz or higher processor clock speed recommended; 233 MHz minimum required (single or dual processor system), Intel Pentium/Celeron family, or AMD K6/Athlon/Duron family, or compatible processor recommended.  
256 megabytes (MB) of RAM or higher recommended (128 MB minimum supported; may limit performance and some features)  
500 MB of available hard disk space  
Super VGA (800 W 600) or higher-resolution video adapter and monitor  
CD-ROM or DVD drive  
One free COM port  
Keyboard and mouse are required.